

1/6

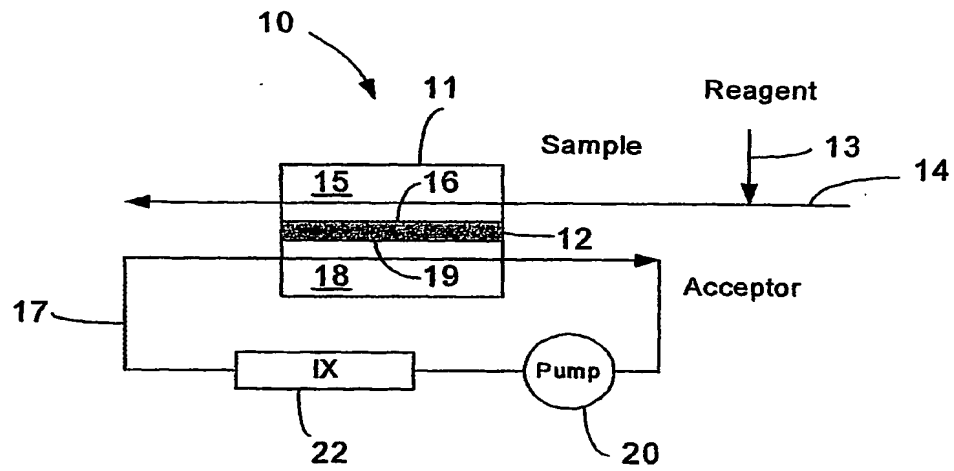


Fig.1

2/6

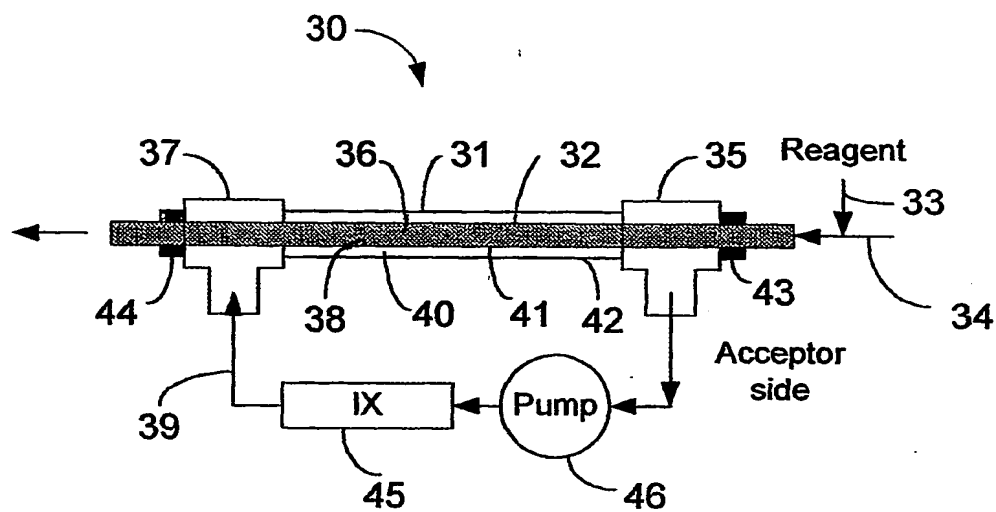


Fig.2

3/6

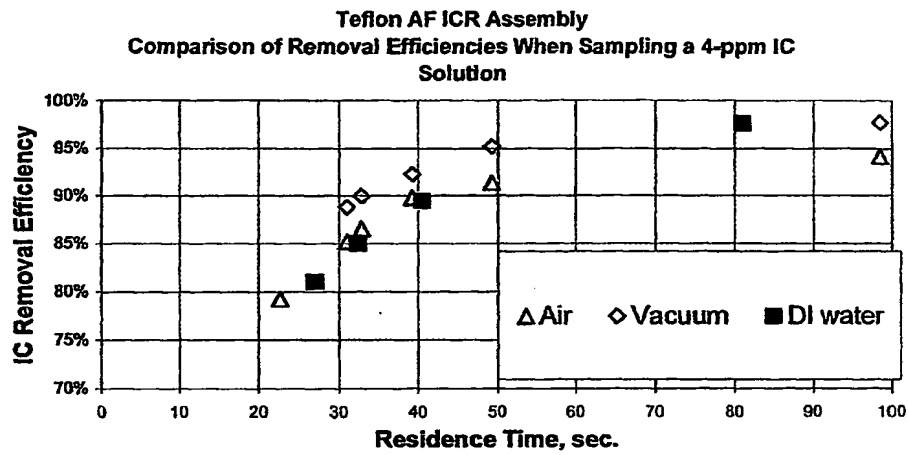
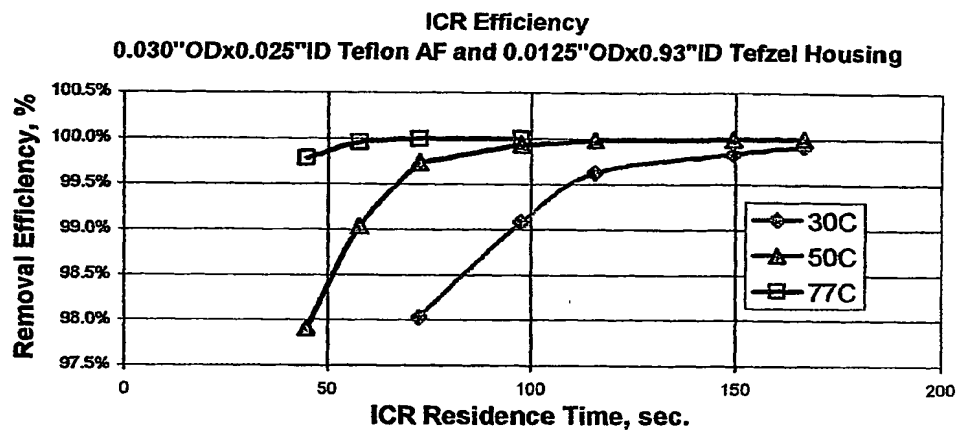


Fig.3

4/6

**Fig. 4**

5/6

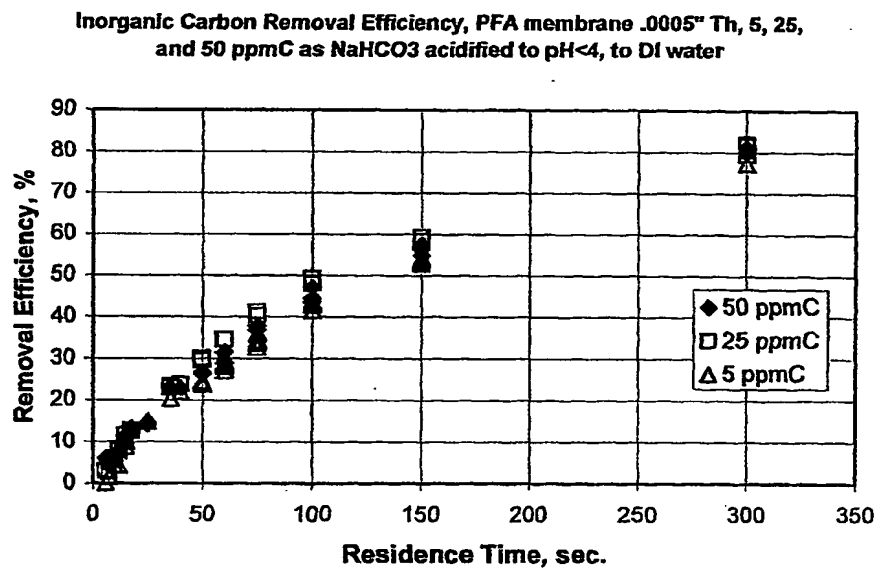


Fig.5

6/6

Volatile Loss with Teflon AF and Gortex, 15 sec. Residence time

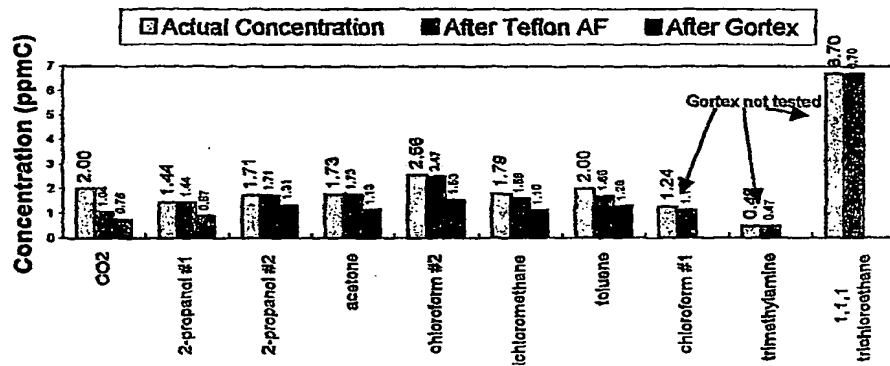


Fig.6